Go To Table Of Contents

Ritter®

Installation and Operation Manual

109 Pediatric Table

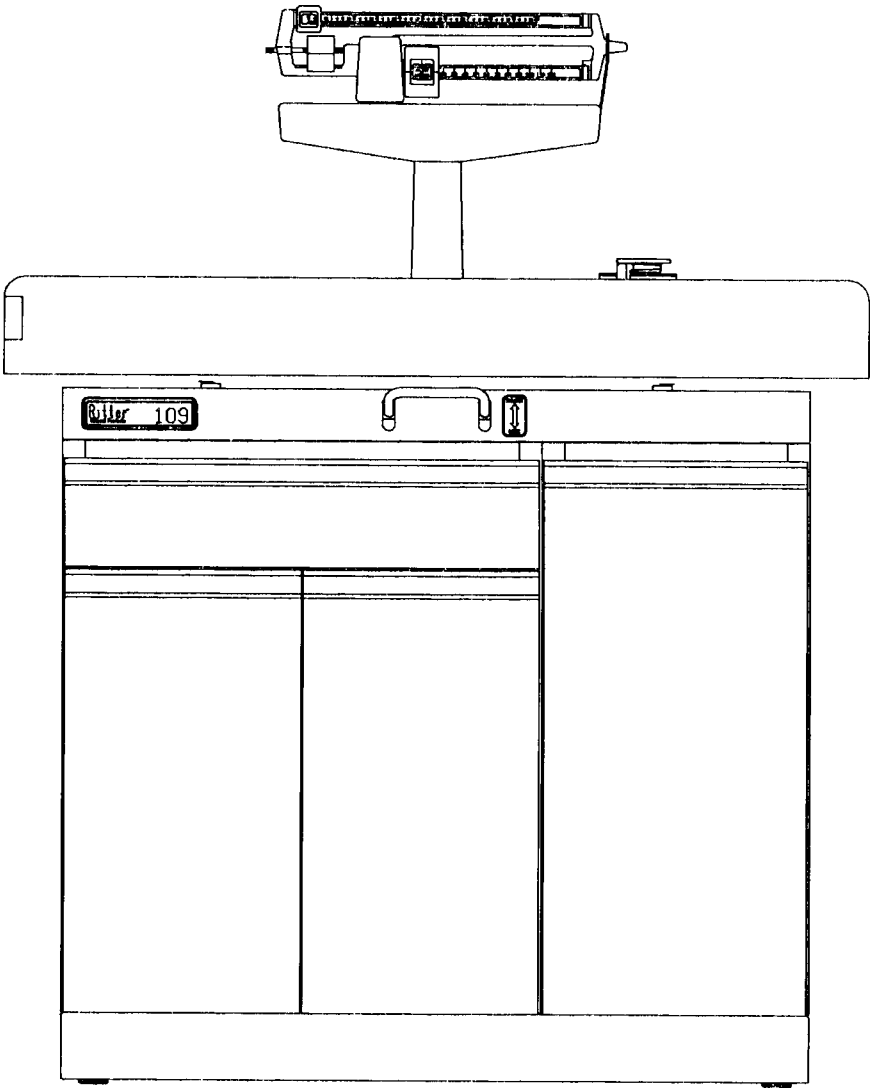

Go To Table Of Contents

Go To Table Of Contents

FOR YOUR PROTECTION

THESE GOODS LEFT OUR FACTORY IN PERFECT ORDER and we hold the Carrier's Receipt for them in this condition.

IF THESE GOODS ARE DAMAGED in Transit, such damaged goods should either be refused, or not accepted until the Transportation Company's Agent has noted on the freight bill, which he will give you, the nature and extent of the damage. He is required to do this. In the same manner, if any goods are LOST in transit, have the shortage noted on the freight bill by the agent.

CONCEALED DAMAGE. If there should be damage of such nature that it could not be detected until the goods were unpacked have the Transportation Company's Agent call AT ONCE and inspect them. Require him to give you a "concealed" bad order report, stating the condition of the goods when examined. It is his duty to do this and you should INSIST upon it.
IF THE ABOVE INSTRUCTIONS ARE COMPLIED WITH we shall cheerfully render all possible assistance in establishing claims against the Transporation Companies for loss and damage in transit.

WE DO NOT ACCEPT GOODS RETURNED FOR CREDIT, EXCHANGE, REPAIRS or for any other reason, unless you have first communicated with us and secured our written permission.

Important Instructions

Safety First: The primary concern of Midmark Corporation is that this equipment be operated and maintained with the safety of the patient and doctor in mind. To assure safer and more reliable operation:

1. Read this manual before installing or operating your equipment.
2. It is the responsibility of the purchaser to assure that appropriate personnel are informed of the contents of this manual.
3. Be sure that you understand the instructions contained in this manual before attempting to install or operate this table.
4. This manual should remain permanently affixed to the equipment.

Warnings

Throughout this manual are Note, Caution, and Danger warnings that call attention to particular procedures. The items are used as follows:

Note
A note is used to amplify an operating procedure, practice, or condition.

CAUTION
A CAUTION is used for an operating procedure, practice, or condition which, if not correctly followed, could result in equipment damage.

DANGER
A DANGER is used for an operating procedure, practice, or condition which, if not correctly followed, could result in personal damage.

DANGER warnings are repeated here. Become thoroughly familar with them and observe them at alL times.

DANGER
Lifting the table while holding the upholstered top, doors, or panels could cause personal injury or damage to the table.

DANGER
Failure to make only light contact with the patient when using the measuring arm could result in personal injury.

Contents

Important Instructions 1
Maintenance 2

General Operation
1. Unpacking 3
2. Installation of Shelves 3
3. Leveling 3
4. Operation of Table Features 3
5. Care of Table 4

General Operation and Care of Equipment Introduction

This manual covers complete instructions for the installation, operation, and normal care of Model 109 Pediatric Examination Table.

Maintenance

See Scale Manufacturer's instruction book for any scale maintenance.

109 Pediatric Examination Table

Unpacking: To avoid damaging the table's upholstered top or side panels, do not use a knife or other sharp object to open the packaging when unpacking. Using a 1/2" wrench, unbolt the table from the wooden shipping skid by removing four bolts located on opposite corners on the underside of the base. After unbolting, remove the table from the skid. Lift by opening the drawer and door and grasping the upper wrap front and back. Do not lift by holding onto the upholstered top, doors, drawers or laminated panels.

Installation of Shelves: Install shelves to desired height in storage areas by installing brackets in four standards and placing shelves on brackets. Check that shelves are level and secure before using.

Leveling: A leveling screw is located under each corner of the table base. By adjusting these in or out, a level, solid installation can be achieved on uneven floors.

CAUTION
Using a knife or other sharp objects to open the packaging could cause equipment damage.

DANGER
Lifting the table while holding the upholstered top, doors, or panels could cause personal injury or damage to the table.

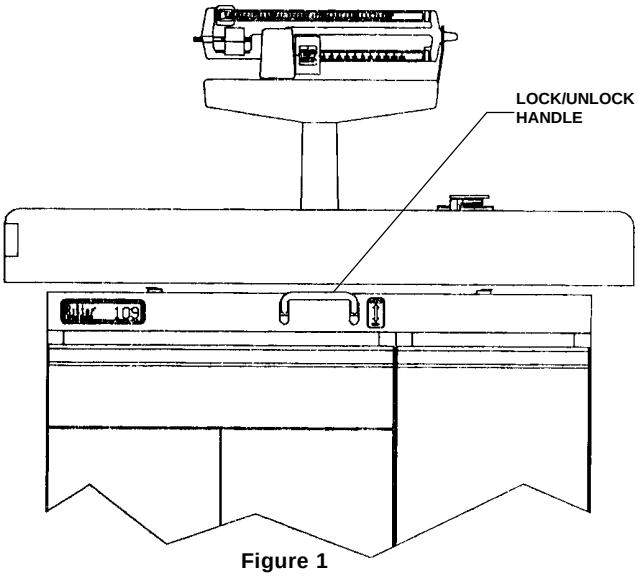

Figure 1

Operation of Table Features

Examination of Patients: All examinations should be done with the table's LOCK/UNLOCK Handle in the LOCK position. (See Figure 1) The table should be in the UNLOCK position for weighing only.

Use of Length Scale: Pull measuring arm away from back of table and slide to right to give clearance for patient. Place patient on table with feet at left end against stop. Keeping the patient extended, slide the measuring arm back until it makes contact with the patient's head. Make only light contact and avoid swinging the arm into the patient. Read the patient's length at the arrow on the pivot end of the arm. (See Figure 2)

DANGER
Failure to make only light contact with the patient when using the measuring arm could result in personal injury.

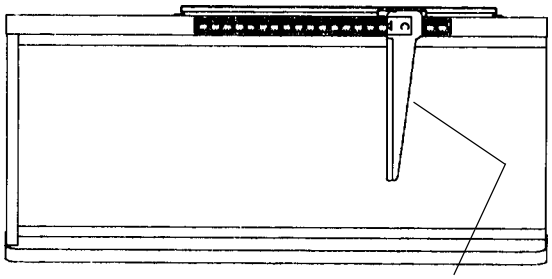

Figure 2

Use of Weight Scale: (Not applicable on all tables). See Scale Manufacturer's instructions for Scale Assembly and Operation.

After scale has been completely assembled remove thumbscrew located on bottom of scale.

Table is provided with a LOCK/UNLOCK Handle. Place the handle in the LOCK position for patient examination. Table top will be secure in the LOCK position.

Place handle in the UNLOCK position for weighing. After weighing return handle to the LOCK position.

Note
Off center placement of the patient will result in inaccurate scale readings. Place patient in approximate center of top for weighing.

Scale balance should be checked periodically, Unlock the scale then press firmly down on table top several times to seat scale mechanism. Adjust readings as required (See Manufacturer's instructions on Zero Adjustment).

Paper Roll: An area under the left-hand side of the top will accept a paper roll up to 18" wide x 3 1/4" in diameter.

Drawer Removal: Pull drawer out to full extension, grasp with both hands and firmly pull drawer straight out until drawer stop disengages.

Care of Table

Care of Upholstery: The upholstery material used to cover the top of the table is resistant to most medicinal-type stains but may be damaged by solvents and dyes. Regular care should be maintained by daily wiping with a damp cloth or sponge and periodic cleaning with a mild soap and water solution.

Any fluid spilled on the upholstery should be removed as quickly as possible.

In the case of stain, attempt to remove it with soap and water.

Care of Painted Metal Surfaces: All painted metal surfaces should be wiped clean with a clean, soft cloth weekly and periodic applications of paste wax made to all smooth painted surfaces to reserve the finished luster.

Return To Table Of Contents

LIMITED WARRANTY

SCOPE OF WARRANTY

Midmark Corporation (“Midmark”) warrants to the original purchaser its new Alternate Care products and components (except for components not warranted under “Exclusions”) manufactured by Midmark to be free from defects in material and workmanship under normal use and service. Midmark’s obligation under this warranty is limited to the repair or replacement, at Midmark’s option, of the parts or the products the defects of which are reported to Midmark within the applicable warranty period and which, upon examination by Midmark, prove to be defective.

APPLICABLE WARRANTY PERIOD

The applicable warranty period, measured from the date of delivery to the original user, shall be one (1) year for all warranted products and components.

EXCLUSIONS

This warranty does not cover and Midmark shall not be liable for the following: (1) repairs and replacements because of misuse, abuse, negligence, alteration, accident, freight damage, or tampering; (2) products which are not installed, used, and properly cleaned as required in the Midmark “Installation” and or “Installation / Operation Manual for this applicable product. (3) products considered to be of a consumable nature; (4) accessories or parts not manufactured by Midmark; (5) charges by anyone for adjustments, repairs, replacement parts, installation, or other work performed upon or in connection with such products which is not expressly authorized in writing in advance by Midmark.

EXCLUSIVE REMEDY

Midmark’s only obligation under this warranty is the repair or replacement of defective parts. Midmark shall not be liable for any direct, special, indirect, incidental, exemplary, or consequential damages or delay, including, but not limited to, damages for loss of profits or loss of use.

NO AUTHORIZATION

No person or firm is authorized to create for Midmark any other obligation or liability in connection with the products.

THIS WARRANTY IS MIDMARK’S ONLY WARRANTY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED. MIDMARK MAKES NO IMPLIED WARRANTIES OF ANY KIND INCLUDING ANY WARRANTIES OF MERCHANTABILITY OR FITNESS FOR ANY PARTICULAR PURPOSE. THIS WARRANTY IS LIMITED TO THE REPAIR OR REPLACEMENT OF DEFECTIVE PARTS.

SF-1487 REV. A1

Return To Table Of Contents

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
937-526-3662 TELEX 288007 FAX 937-526-5542

© Midmark Corporation - 1996